

Shaping Ability of HyFlex EDM and ProTaper Next Rotary Instruments in Curved Root Canals: A Micro-CT Study

Ahmed K Turkistani¹, Madiha M Gomaa², Lubna A Shafei³, Loai Alsofi⁴, Abdul Majeed⁵, Emad AlShwaimi⁶

ABSTRACT

Aim: The aim of this study is to evaluate and compare the shaping ability of HyFlex™ EDM (HFEDM) and ProTaper Next (PTN) rotary instruments in curved root canals by using micro-computed tomography (micro-CT) imaging.

Materials and methods: A total of 22 mandibular molar teeth having separate mesial canals with 20 to 30° curvatures were randomly divided into two groups and instrumented with HFEDM (OneFile) or PTN (X1 and X2). Pre- and post-instrumentation micro-CT scans were obtained. Mesiodistal canal transportation and centering ability were evaluated in four cross-sections (2, 4, 6, and 8 mm from apex). Changes in canal volume and surface area were measured for a 10-mm standardized area of interest. Kolmogorov–Smirnov and Shapiro–Wilk tests were used to assess the normality and homogeneity. Independent and paired *t* tests and one-way ANOVA were used to analyze data at the $p < 0.05$ level.

Results: Compared to PTN, HFEDM showed significantly less mesiodistal canal transportation and improved centering ability in cross-section L6 ($p < 0.05$). The instruments showed similar increases in volume and surface area of the canals, with minor insignificant differences.

Conclusion: HFEDM and PTN files were safe to use in curved canals and showed similar shaping ability, while respecting the original anatomies. HFEDM OneFile performed better at the vicinity of the danger zone in terms of mesiodistal canal transportation and centering ability.

Keywords: Canal transportation, Centering ability, Curved canal, HyFlex EDM, Micro computed tomography, ProTaper Next.

The Journal of Contemporary Dental Practice (2019): 10.5005/jp-journals-10024-2579

INTRODUCTION

Canal shaping in root canal treatment is a strategic phase aimed at removing pulp remnants, necrotic tissues, microorganisms, and debris, to prepare the canal for 3D root filling.¹ The shaping process should respect the original canal anatomy without changing the position of the apical foramen or excessively weakening the root.² However, canal transportation, zipping, ledging, or stripping can occur during preparation when using manual or rotary instrumentation techniques. Although NiTi rotary files reportedly maintain the original canal anatomy better than stainless-steel hand files,^{3,4} instrumentation of severely curved canals remains challenging for most endodontic practitioners.⁵

To enhance the mechanical properties, performance, and safety of NiTi instruments, manufacturers have developed several new technologies, such as M-wire, R-phase, and the newly introduced controlled memory (CM) and proprietary thermal technology.⁶ Thermal metallurgical processing and new instrument cross-sectional designs are considered major developments. ProTaper Next (PTN) (Dentsply Maillefer, Ballaigues, Switzerland) and HyFlex EDM (HFEDM) (Coltène/Whaledent, Altstätten, Switzerland) are examples of the latest generation of rotary instruments.

PTN is made of M-wire alloy and has an offset design, producing a “swaggering” effect. M-wire has higher flexibility and cyclic fatigue resistance than conventional NiTi.^{2,7} Silva et al.⁸ reported that PTN produced canal preparations that were more centered and had slightly higher apical transportation than canals produced by ProTaper Universal or WaveOne rotary instruments in simulated artificial curved canals. An off-centered rectangular cross-section with variable taper design (increasing to decreasing in the apicocoronal direction) reportedly enhances flexibility and debris removal, reduces engagement, and limits taper lock, screwing, and torque on any given file.⁹

^{1–4}Department of Endodontics, Faculty of Dentistry, King Abdulaziz University, Jeddah, Saudi Arabia

^{5,6}Division of Endodontic, Department of Restorative Dental Sciences, College of Dentistry, Imam Abdulrahman Bin Faisal University, Dammam, Saudi Arabia

Corresponding Author: Loai Alsofi, Department of Endodontics, Faculty of Dentistry, King Abdulaziz University, Jeddah, Saudi Arabia, Phone: +966 555318481, e-mail: lalsofi@kau.edu.sa

How to cite this article: Turkistani AK, Gomaa MM, et al. Shaping Ability of HyFlex EDM and ProTaper Next Rotary Instruments in Curved Root Canals: A Micro-CT Study. *J Contemp Dent Pract* 2019;20(6):680–685.

Source of support: Nil

Conflict of interest: None

HFEDM is a third-generation single file that was introduced with an innovative manufacturing process using electric discharge machining (EDM) followed by CM treatment. CM is a proprietary metallurgical thermal treatment that reduces the shape memory of NiTi files¹⁰ and enhances the flexibility and cyclic fatigue resistance of instruments.^{11,12} The cross-sectional design of HFEDM instruments is variable, rectangular toward the tip and roughly triangular toward the shaft. In previous studies, these instruments showed very high resistance to cyclic fatigue compared to instruments produced by CM technology and M-wire.^{11,13,14}

Numerous investigations have compared PTN to single-file systems; however, to the authors' knowledge, no study has investigated the shaping ability of the newly introduced HFEDM OneFile (25/0.08) in severely curved root canals. Therefore, the purpose of this study was to compare the shaping abilities of HFEDM and PTN rotary instruments in curved root canals by micro-computed tomography (micro-CT). The null hypothesis was that

there would be no difference in shaping ability between these instruments.

METHODOLOGY

A total of 22 human mandibular first and second molars were selected from a pool of freshly extracted teeth. Selection criteria were as follows: teeth extracted for periodontal, prosthetic, or orthodontic reasons, having unfused mesial and distal roots, curved mesial roots, and mature apices. Teeth with root cracks, fractures, or external root resorption as confirmed by magnifying loops were excluded.

After being cleaned of debris and tissue remnants, teeth were placed in 5.25% NaOCl solution for 30 minutes. Digital radiographs of each tooth were taken at a standard position from the buccal and mesial views with a Heliodont MD X-ray unit (Siemens, Bensheim, Germany). Root curvature angles were measured in the buccolingual plane by using Image J software (Fiji) for teeth with a type IV "Vertucci" canal configuration. Teeth having moderate curvatures of 20–30° in mesial roots were included in the study. Teeth were stored in 0.1% thymol solution at 5 °C in separately labeled containers until time of use.

Specimen Preparation

All teeth preparation was conducted at the Faculty of Dentistry, King Abdulaziz University, Jeddah, Saudi Arabia. Straight-line access cavities were prepared in each tooth by high-speed diamond burs. Specimens were adjusted to a standard length of 18 ± 1 mm by decapitating crowns from the occlusal surfaces while using diamond discs under copious water-cooling. Patency of mesial canals was confirmed. An ISO size-10 K-file was inserted into the canal until it was observed at the apical foramen. Working length (WL) was calculated by subtracting 0.5 mm from that length. A smooth reproducible glide path was produced by using hand K-files up to size 15. The coronal 2 mm was preflared with size 1 and 2 Gates-Glidden drills (Dentsply Maillefer) in a crown-down manner. Specimens were randomly divided into two groups of 22 canals each and instrumented as follows. Each group included 11 mesiobuccal canals and 11 mesiolingual canals.

Group 1: HFEDM

According to the manufacturer's guidelines, HyFlex (25/0.08) OneFile was used to shape the root canal up to WL by the crown-down technique with full clockwise rotation. The X Smart Plus (Dentsply Maillefer) endodontic motor was used with a 16:1 reduction handpiece, a rotational speed of 400 RPM, and 2.5 N cm torque, as recommended by the manufacturer.

Group 2: PTN

ProTaper Next X1 (17/0.04) and X2 (25/0.06) files were used for shaping canals with a 16:1 reduction handpiece. The handpiece was powered by a preprogrammed X Smart Plus motor, which was set at 300 RPM and 4 N cm torque, according to the manufacturer's recommendations. The X1 file was used in a brushing motion, followed by irrigation and recapitulation before insertion of X2 to the full WL.

In both groups, a new file was used to prepare each canal. Canals were irrigated with 2 mL of 2.5% sodium hypochlorite (NaOCl) solution before and during instrumentation by using a 30-gauge side-vented needle (Hawe irrigation probe, Bioggio, Switzerland) in an intermittent manual flush technique. After instrumentation, canals were irrigated with 5 mL of 2.5% NaOCl followed by 5 mL of 17% ethylene-diamine-tetra-acetic acid (EDTA) applied for

60 seconds. Canals were rinsed with 2 mL of distilled water and dried with paper points.

Micro-CT Scanning and Study Parameter Calculations

All micro CT scanning and analysis were conducted at the College of Dentistry, Imam Abdulrahman Bin Faisal University, Dammam, Saudi Arabia. After resection of the distal roots, each sample was mounted in a custom-made resin holder (1 cm deep \times 2 cm wide). Pre- and post-instrumentation images were scanned by using a SkyScan 1172 micro-CT scanner (Bruker, Luxemburg, Belgium) at a resolution of 8.99 μ m. The volume of interest was set at 10 mm from the apical foramen for all specimens.¹⁵ Images were reconstructed by NRecon Software (Bruker). Scanned images were evaluated for pre- and post-instrumentation at predetermined root canal cross-sections (2, 4, 6, and 8 mm from apex). The shaping ability was evaluated according to canal volume, surface area, transportation, and centering ability.

Canal Volume and Surface Area

Raw images of cross-section slices were reconstructed with SkyScan's NRecon version 1.6.4 software (Bruker) and saved as bitmap image (BMP) format. Then CTan v1.11.10.0 software (Bruker) was used for three-dimensional image reconstruction and measurement of the volume and surface area. The changes in root canal volume ($\Delta V/\text{mm}^3$) and surface area ($\Delta S/\text{mm}^2$) were calculated by subtraction of the pre- and post-instrumentation values and compared between the two tested shaping techniques.

Canal Transportation

Canal transportation was determined in the mesiodistal direction. Where X1 reveals the amount of dentin before instrumentation and X2 reveals the amount after instrumentation. Y1 reveals the distance from the furcation of the curved root to the periphery of the uninstrumented canal and Y2 reveals the distance from the inside of the curved root to the periphery of the instrumented canal. Mesial (X, Y) and distal (X, Y) dentin thicknesses were measured from pre- and post-instrumentation images in both groups at the four cross-sectional levels (2, 4, 6, and 8 mm from apex). Canal transportation at each level was calculated as described by Gambill et al.,¹⁶ (Fig. 1), using the following equation: $[(X1 - X2) - (Y1 - Y2)]$. A transportation

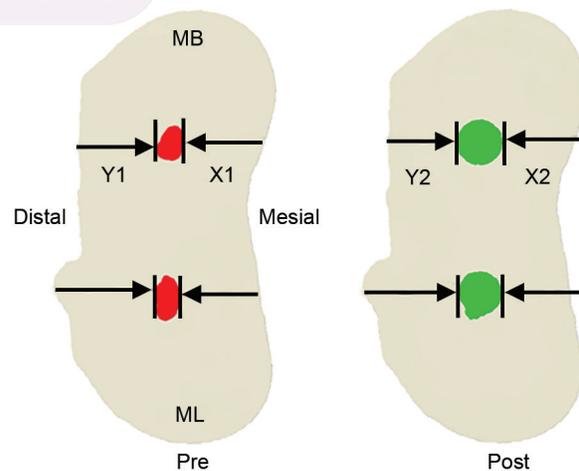


Fig. 1: Representative micro-CT coronal plane sample of a pre- and post-instrumentation depicting the measurement of mesial and distal dentin thicknesses according to Gambill et al.¹⁶

value of zero indicates no transportation; a positive value indicates transportation directed to the mesial side; and a negative value indicates transportation to the distal side of the canal.¹⁶

Centering Ability

Canal centering ability was determined in the mesiodistal direction at each cross-sectional level, by using the following equation:¹⁶ $[(X1 - X2)/(Y1 - Y2)]$ or $[(Y1 - Y2)/(X1 - X2)]$. A centering ratio of one indicates perfect centering. The closer the ratio is to zero, the worse the ability of the instrument to maintain itself in the central axis of the canal (Fig. 1). The centering ability was defined as the ability of the file to remain in the center of the canal during the shaping cycle.¹⁶

Statistical Analysis

Data were analyzed by using the SPSS ver. 22 software package (SPSS Inc, Chicago, IL, USA). Kolmogorov–Smirnov and Shapiro–Wilk

tests were used to assess normality of the data distributions. Data were presented as means \pm standard deviations (SDs). Independent *t* tests were used to compare changes in volume, surface area, canal transportation, and centering ability between groups. Paired *t* test and one-way ANOVA for repeated measures were used to compare within groups for comparisons of more than two variables. The significance level was set at $p < 0.05$.

RESULTS

No instrument fractured during instrumentation in either group. Figure 1 shows representative micro-CT coronal plane sample of a pre- and post-instrumentation depicting the measurement of mesial and distal dentin thicknesses. Figure 2 shows the composite photograph of representative micro-CT coronal planes of superimposed samples. Pre-instrumentation canals are shown in red and post-instrumentation in green. In this sample, the upper canal (MB) was prepared by PTN X1 and X2 and the lower canal (ML) by HFEDM OneFile. Various degrees of transportation and centering ability can be seen at different cross-sections. Figure 3 shows representative micro-CT images A–C of the mesial root of a mandibular molar in mesiodistal direction: canals before instrumentation (A), after instrumentation (B), and superimposed pre- and post-instrumentation images (C). Mesio Buccal canal was prepared by PTN X1 and X2 and the mesiolingual canal by HFEDM OneFile. In the three-dimensional images, original canal anatomy is depicted in red and shape produced by instrumentation is shown in green. Images D–E depict three-dimensional reconstruction of MB and ML canals from occlusal plane.


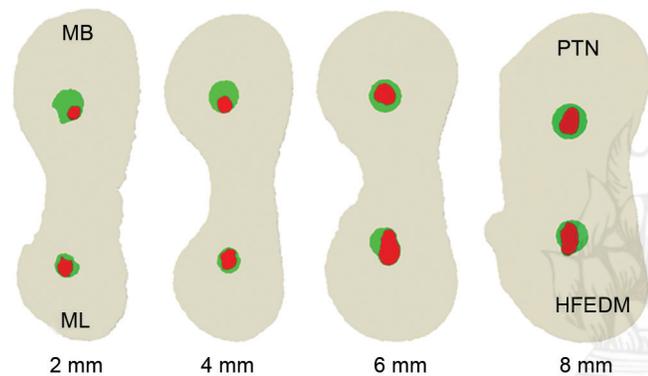


Fig. 2: Composite photograph of representative micro-CT coronal planes of superimposed samples. Pre-instrumentation canals are shown in red and post-instrumentation in green. In this sample, the upper canal (MB) was prepared by PTN X1 and X2 and the lower canal (ML) by HFEDM OneFile. Various degrees of transportation and centering ability can be seen at different cross-sections

Canal Volume and Surface Area

Table 1 shows means and SDs for changes in root canal volume and surface area in both groups. Canal volume and surface area were higher after instrumentation than they were before instrumentation in both groups ($p < 0.05$). HFEDM produced greater changes in canal volume and surface area than PTN, but these differences were not significant.

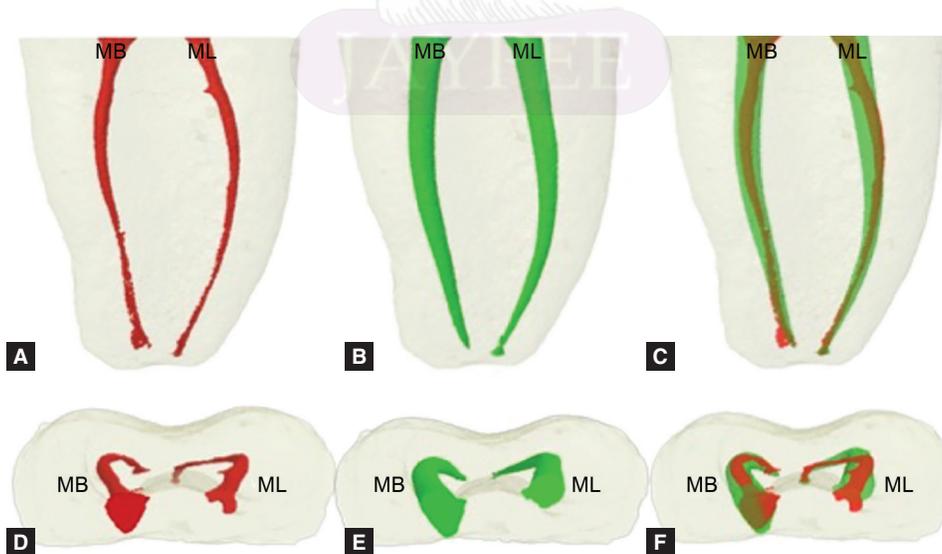

Figs 3A to E: Representative micro-CT images (A–C) of the mesial root of a mandibular molar in mesiodistal direction. (A) Canals before instrumentation; (B) After instrumentation; and (C) Superimposed pre- and post-instrumentation images. Mesio Buccal canal was prepared by PTN X1 and X2 and the mesiolingual canal by HFEDM OneFile. In the three-dimensional images, original canal anatomy is depicted in red and shape produced by instrumentation is shown in green. Images (D–E) depict three-dimensional reconstruction of MB and ML canals from occlusal plane

Table 1: Changes (mean \pm SD) in canal volume (mm³) and surface area (mm²) with different file systems

Groups	Volume change (ΔV)	Surface area change (ΔS)
HFEDM	2.689 \pm 0.815	7.773 \pm 3.849
PTN	2.326 \pm 0.911	6.690 \pm 4.960

Canal Transportation

Absolute values of the degree of canal transportation are presented in Table 2. Both file systems showed canal transportation at all tested levels ($p < 0.05$); with minimal transportation at the apical end (L2) and maximal transportation toward the coronal end (L8). Canal transportation was comparable between groups at L2, L4, and L8 (Table 2). At L6, lower transportation was detected for HFEDM than was observed for PTN ($p < 0.05$; Table 2). Most canals were transported toward the mesial side apically (+ve) and distal side coronally (–ve), with no significant differences between groups.

Centering Ability

Compared to PTN, HFEDM resulted in a more centered preparation at all tested levels (Table 3). A statistically significant difference was detected at L6, where HFEDM showed the highest centering ability ($p < 0.05$; Table 3). Differences between groups were small and not significant at any other level.

DISCUSSION

The present study evaluated the shaping ability of HFEDM and PTN files in curved canals using micro-CT. Based on the results, the null hypothesis that there is no difference in shaping ability between the two rotary instruments was rejected.

To the authors' knowledge, no study to date has evaluated the shaping ability of newly introduced HFEDM files in narrow curved canals. In a recent *in vitro* study, Venino et al.¹⁷ investigated the shaping ability of HFEDM and PTN files. They considered both straight and wide canals of single- and multi-rooted teeth. Therefore, the results could not be compared directly to those of the present study, in which narrow and curved root canals were used.

In the present study, mesial roots of mandibular molar teeth with curvatures of 20–30°¹⁸ were used to allow relative standardization of shape and curvature.^{19,20} Such standardization has been recommended as an ideal model to evaluate and compare shaping abilities of different rotary instruments.²¹ Comparable preoperative canal curvatures were utilized in most previous studies evaluating the shaping abilities of NiTi instrument systems.^{22,23} The present

investigation was based on the micro-CT scanning for the evaluation of the shaping ability of tested instruments. This method was recommended previously^{16,24} and has been utilized by numerous studies.^{8,17,25–28} Using a standardized nondestructive method for measurement facilitates later comparison between studies and helps in reaching a generalizable and dependable consensus.

Canal volume and surface area are parallel interdependent parameters that can give a full picture of the ability of a tested instrument to shape a larger volume and surface area, in terms of being gradually tapered and amenable for three-dimensional obturation.^{8,26,29,30} The HFEDM group showed slightly greater changes in volume and surface area than the PTN group, but the differences were not significant. The HFEDM single file increased the canal volume and surface area to comparable levels as provided by the combined PTN X1 (#17/0.04) and X2 (#25/0.06) instrumentation. Previous studies comparing single-file systems (e.g., WaveOne Primary and OneShape) with PTN reported similar findings,^{31,32} although the findings could not be generalized to all single-file designs. Madani et al.³¹ found smaller canal volumes coronally when the NeoNiTi A1 single file was used compared to the ProTaper Universal multifile system.

Canal transportation of varying degrees from 100 to 200 μ m has been observed when root canals are instrumented with rotary instruments.⁵ Relatively less transportation was detected for both rotary instruments in this study, consistent with findings of previous studies evaluating the shaping abilities of HFEDM¹⁷ and PTN.^{2,8,17,27,31} A general trend of increased magnitude of canal transportation in the coronal direction was noted, in accordance with the findings of Gu et al.³³ They found that heat-treated NiTi instruments—specifically, Twisted Files (R-phase), WaveOne (M-wire), HyFlex CM, and V Taper 2H (CM-wire)—showed more transportation at coronal than at apical curvatures.

Statistically significant differences between the two instruments were observed for mesiodistal canal transportation and centering ability only in cross-section L6. This area represents the middle to coronal third of the root canal, where excessive removal of dentin (transportation) could result in weakening of the dentinal wall or stripping perforation.¹⁷ Wu et al.³⁴ reported that transportation of more than 300 μ m could compromise treatment outcomes. However, transportation values obtained here from both instruments were well below this 0.3 mm critical thickness.

Canal transportation and centering ability could be influenced by the flexibility, cross-sectional shape, and taper of instruments.³⁵ PTN X1 and X2 files present a variable taper design, with progressive tapering in the apical section and decreasing taper in the coronal section. HFEDM

Table 2: Transportation (mm) of the canals at different levels after instrumentation with tested files (mean \pm SD)

Groups	Canal transportation (mm from the apex)			
	L2	L4	L6	L8
HFEDM	0.059 \pm 0.045	0.113 \pm 0.102	0.091 \pm 0.068*	0.185 \pm 0.122
PTN	0.068 \pm 0.054	0.095 \pm 0.070	0.137 \pm 0.089*	0.199 \pm 0.119

*Statistical significant difference ($p < 0.05$)

Table 3: Centering ratio of tested files at different measurement levels (mean \pm SD)

Groups	Centering ration (mm from the apex)			
	L2	L4	L6	L8
HFEDM	0.52 \pm 0.30	0.50 \pm 0.32	0.63 \pm 0.19*	0.47 \pm 0.27
PTN	0.39 \pm 0.31	0.47 \pm 0.30	0.37 \pm 0.27*	0.38 \pm 0.25

*Statistical significant difference ($p < 0.05$)

OneFile (#25/0.08) has a decreasing taper design that starts 4 mm from the tip. The L6 cross-section was located 6 mm from the apex, which coincides with the greatest taper of the PTN files. Therefore, the significant difference in transportation observed at L6 could be related to the instrument taper.¹⁷ Similar findings were reported in a study comparing the shaping abilities of the PTN, ProTaper Universal, and WaveOne instruments in L-shaped simulated root canals. PTN maintained the canal curvature with minimal apical transportation and the highest coronal transportation above the curvature.³⁶

Transportation was directed mesially (+ve) at apical sections and distally (-ve) at coronal sections in both groups. PTN showed slightly higher values than HFEDM, but the differences were not significant. It may be that the PTN file has a higher tendency to straighten curved canals and causes transportation toward the furcation at the midcoronal level (distal) and toward the outer aspect of the curvature (mesial) at the apical 1–3 mm. A similar trend was reported for PTN in previous studies.^{25,26,37,38}

HFEDM showed less transportation and better centering ability in all cross-sectional levels, although the difference from the PTN group was not significant. This finding is not surprising and could be related to the greater flexibility of the HFEDM file. Instruments with greater flexibility may be more suitable for the preparation of severely curved root canals.³ CM technology renders HyFlex files more flexible than conventional NiTi and M-wire instruments of similar sizes and tapers.^{12,39} On the one hand, Venino et al.¹⁷ evaluated the shaping abilities of HFEDM and PTN instruments in extracted teeth. Both files respected the original canal anatomy and safely prepared the canals. HFEDM caused slightly less buccolingual transportation and better centering than PTN in the middle and coronal thirds, although canal curvature was not taken into consideration. In the present study, similar shaping behavior was observed for both file systems in severely curved canals. On the other hand, Saber et al.²³ reported that PTN caused significantly greater straightening of severely curved root canals than HyFlex CM and iRaCe instruments. However, the three instruments showed similar apical transportation results.

To our knowledge, the small size was one of the limitations of the study due to cost and financial issues. One drawback was that only transportation in the mesial and distal directions were calculated while omitting the transportation in the buccal and lingual direction.

CONCLUSION

HFEDM OneFile outperformed the PTN multifile system, producing less transportation and better centering at the 6 mm root level. Overall, HFEDM and PTN were safe and effective in curved canals and showed similar shaping ability while maintaining the original canal anatomies. Our results recommend using HFEDM in severely curved canals to avoid strip perforation.

CLINICAL SIGNIFICANCE

Based on the results of the study, it is recommended to use HFEDM in severely curved canals to avoid strip perforation and to maintain original canal curvature.

ACKNOWLEDGMENTS

The authors deny any conflict of interests in this research. The authors would like to thank Mr Lindsay and Mr Jim for their help in micro-CT of the samples.

REFERENCES

- Peters OA. Current challenges and concepts in the preparation of root canal systems: a review. *J Endod* 2004 Aug;30(8):559–667.
- Wei Z, Cui Z, et al. A comparison of the shaping ability of three nickel-titanium rotary instruments: a micro-computed tomography study via a contrast radiopaque technique in vitro. *BMC Oral Health* 2017 Jan 9;17(1):39. DOI: 10.1186/s12903-016-0326-5.
- Pereira ES, Viana AC, et al. Behavior of nickel-titanium instruments manufactured with different thermal treatments. *J Endod* 2015 Jan;41(1):67–71. DOI: 10.1016/j.joen.2014.06.005.
- Alrahabi M. Comparative study of root-canal shaping with stainless steel and rotary NiTi files performed by preclinical dental students. *Technol Health Care* 2015;23(3):257–265. DOI: 10.3233/THC-150895.
- Hülsmann M, Peters OA, et al. Mechanical preparation of root canals: shaping goals, techniques and means. *Endod Topics* 2005 Marh;10(1):30–76.
- Ye J, Gao Y. Metallurgical characterization of M-Wire nickel-titanium shape memory alloy used for endodontic rotary instruments during low-cycle fatigue. *J Endod* 2012 Jan;38(1):105–107. DOI: 10.1016/j.joen.2011.09.028.
- Gao Y, Gutmann JL, et al. Evaluation of the impact of raw materials on the fatigue and mechanical properties of ProFile Vortex rotary instruments. *J Endod* 2012 Mar;38(3):398–401. DOI: 10.1016/j.joen.2011.11.004.
- Silva EJ, Vieira VC, et al. Quantitative transportation assessment in curved canals prepared with an off-centered rectangular design system. *Braz Oral Res* 2016;30(1):e43. DOI: 10.1590/1807-3107.
- Ruddle CJ, Machtou P, et al. The shaping movement: fifth-generation technology. *Dent Today* 2013 Apr;32(4):94, 96–99.
- Zhao D, Shen Y, et al. Micro-computed tomography evaluation of the preparation of mesiobuccal root canals in maxillary first molars with Hyflex CM, Twisted Files, and K3 instruments. *J Endod* 2013 Mar;39(3):385–388. DOI: 10.1016/j.joen.2012.11.030.
- Pirani C, Iacono F, et al. HyFlex EDM: superficial features, metallurgical analysis and fatigue resistance of innovative electro discharge machined NiTi rotary instruments. *Int Endod J* 2016 May;49(5):483–493. DOI: 10.1111/iej.12470.
- Testarelli L, Plotino G, et al. Bending properties of a new nickel-titanium alloy with a lower percent by weight of nickel. *J Endod* 2011 Sep;37(9):1293–1295. DOI: 10.1016/j.joen.2011.05.023.
- Kaval ME, Capar ID, et al. Evaluation of the cyclic fatigue and torsional resistance of novel nickel-titanium rotary files with various alloy properties. *J Endod* 2016 Dec;42(12):1840–1843. DOI: 10.1016/j.joen.2016.07.015.
- Pedulla E, Lo Savio F, et al. Torsional and cyclic fatigue resistance of a new nickel-titanium instrument manufactured by electrical discharge machining. *J Endod* 2016 Jan;42(1):156–159. DOI: 10.1016/j.joen.2015.10.004.
- Moore J, Fitz-Walter P, et al. A micro-computed tomographic evaluation of apical root canal preparation using three instrumentation techniques. *Int Endod J* 2009 Dec;42(12):1057–1064. DOI: 10.1111/j.1365-2591.2009.01626.x.
- Gambill JM, Alder M, et al. Comparison of nickel-titanium and stainless steel hand-file instrumentation using computed tomography. *J Endod* 1996 Jul;22(7):369–375. DOI: 10.1016/S0099-2399(96)80221-4
- Venino PM, Citterio CL, et al. A micro-computed tomography evaluation of the shaping ability of two nickel-titanium instruments, HyFlex EDM and ProTaper Next. *J Endod* 2017 Apr;43(4):628–632. DOI: 10.1016/j.joen.2016.11.022.
- Schneider SW. A comparison of canal preparations in straight and curved root canals. *Oral Surg Oral Med Oral Pathol* 1971 Aug;32(2):271–275.
- Paque F, Barbakow F, et al. Root canal preparation with Endo-Eze AET: changes in root canal shape assessed by micro-computed tomography. *Int Endod J* 2005 Jul;38(7):456–464.

20. Iqbal MK, Firic S, et al. Comparison of apical transportation between ProFile™ and ProTaper™ NiTi rotary instruments. *Int Endod J* 2004 Jun;37(6):359–364.
21. Paque F, Zehnder M, et al. Microtomography-based comparison of reciprocating single-file F2 ProTaper technique versus rotary full sequence. *J Endod* 2011;37:1394–1397. DOI: 10.1016/j.joen.2011.06.031.
22. Barbosa-Ribeiro M, Albergaria SJ, et al. Canal transportation and centering ability of curved root canals prepared using rotary and reciprocating systems. *Braz J Oral Sci* 2015 Sep;14(3):214–218.
23. Saber SE, Nagy MM, et al. Comparative evaluation of the shaping ability of ProTaper Next, iRaCe and Hyflex CM rotary NiTi files in severely curved root canals. *Int Endod J* 2015 Feb;48(2):131–136. DOI: 10.1111/iej.12291.
24. Peters OA, Laib A, et al. Three-dimensional analysis of root canal geometry by high-resolution computed tomography. *J Dent Res* 2000 Jun;79(6):1405–1409. DOI: 10.1177/00220345000790060901.
25. Elnaghy AM, Elsaka SE. Evaluation of root canal transportation, centering ratio, and remaining dentin thickness associated with ProTaper Next instruments with and without glide path. *J Endod* 2014 Dec;40(12):2053–2056. DOI: 10.1016/j.joen.2014.09.001.
26. Capar ID, Ertas H, et al. Comparative study of different novel nickel–titanium rotary systems for root canal preparation in severely curved root canals. *J Endod* 2014 Jun;40(6):852–856. DOI: 10.1016/j.joen.2013.10.010.
27. Zhao D, Shen Y, et al. Root canal preparation of mandibular molars with 3 nickel–titanium rotary instruments: a micro-computed tomographic study. *J Endod* 2014 Nov;40(11):1860–1864. DOI: 10.1016/j.joen.2014.06.023.
28. Lim YJ, Park SJ, et al. Comparison of the centering ability of Wave-One and Reciproc nickel–titanium instruments in simulated curved canals. *Restor Dent Endod* 2013 Feb;38(1):21–25. DOI: 10.5395/rde.2013.38.1.21.
29. Bürklein S, Börjes L, et al. Comparison of preparation of curved root canals with Hyflex CM and Revo-S rotary nickel–titanium instruments. *Int Endod J* 2014 May;47(5):470–476. DOI: 10.1111/iej.12171.
30. Bürklein S, Hinschitzka K, et al. Shaping ability and cleaning effectiveness of two single-file systems in severely curved root canals of extracted teeth: Reciproc and WaveOne versus Mtwo and ProTaper. *Int Endod J* 2012 May;45(5):449–461. DOI: 10.1111/j.1365-2591.2011.01996.x.
31. Madani Z, Soleymani A, et al. Transportation and centering ability of Neoniti and ProTaper Instruments; A CBCT assessment. *Iran Endod J* 2017 Winter;12(1):43–49. DOI: 10.22037/iej.2017.09.
32. Ghobashy A, Nagy M, et al. Shaping ability of single versus multi file rotary Ni–Ti systems in curved root canals. *Tanta Dent J* 2016 Apr 1;13(2):68.
33. Gu Y, Kum KY, et al. Various heat-treated nickel–titanium rotary instruments evaluated in S-shaped simulated resin canals. *J Dent Sci* 2017 Mar 1;12(1):14–20. DOI: 10.1016/j.jds.2016.04.006.
34. Wu MK, Fan B, et al. Leakage along apical root fillings in curved root canals. Part i: effects of apical transportation on seal of root fillings. *J Endod* 2000 Apr;26(4):210–216. DOI: 10.1097/00004770-200004000-00003.
35. Olivieri JG, Stöber E, et al. In vitro comparison in a manikin model: increasing apical enlargement with K3 and K3XF rotary instruments. *J Endod* 2014 Sep;40(9):1463–1467. DOI: 10.1016/j.joen.2014.02.023.
36. Wu H, Peng C, et al. Shaping ability of ProTaper Universal, WaveOne and ProTaper Next in simulated L-shaped and S-shaped root canals. *BMC Oral Health* 2015 Mar 1;15:27. DOI: 10.1186/s12903-015-0012-z.
37. Ferrara G, Taschieri S, et al. Comparative evaluation of the shaping ability of two different nickel–titanium rotary files in curved root canals of extracted human molar teeth. *J Investig Clin Dent* 2017 Feb;8(1):1–9. DOI: 10.1111/jicd.12187.
38. Celikten B, Uzuntas CF, et al. Comparative evaluation of shaping ability of two nickel–titanium rotary systems using cone beam computed tomography. *BMC Oral Health* 2015 Mar 10;15:32. DOI: 10.1186/s12903-015-0019-5.
39. Pongione G, Pompa G, et al. Flexibility and resistance to cyclic fatigue of endodontic instruments made with different nickel–titanium alloys: a comparative test. *Ann Stomatol (Roma)* 2012 Jul;3(3–4):119–122.

